

Bulk Current Injection Probe

1 Introduction

The TBBCI1-200K280 is a snap-on Bulk Current Injection probe, expanding the Tekbox product range of affordable EMC pre-compliance test equipment.

The BCI probe has been designed primarily for conducted immunity testing in the frequency range 150 kHz to 230 MHz, according to standard IEC / EN 61000-4-6. The insertion loss is 8 dB for most of its bandwidth and it is fully compliant with the insertion loss specification of IEC / EN 61000-4-6. The probe is individually characterized and usable in the frequency range 10 kHz – 300 MHz. It can inject severity levels 1, 2, 3 and level X up to 30V into a conducted immunity test set-up according to IEC/EN 61000-4-6.

The probe can also be used for RF current monitoring applications.



Picture 1: TBBCI1-200K280 Bulk Current Injection probe

The aperture of the RF current monitoring probe is 27 mm. The typical insertion loss is 8 dB and the typical transfer impedance is 26 dB Ohm.

Bulk Current Injection Probe

2 Specification

Compliance:	IEC / EN 61000-4-6 insertion loss specification for BCI clamps
Characterized freq. range:	10 kHz to 300 MHz
Insertion loss:	8 dB typ.; 50 Ohm system (100 Ω loop impedance)
Transfer impedance:	26 dB Ohm typ.; 50 Ohm system (100 Ohm loop impedance)
Power rating:	capable of injecting level 1, 2, 3 and stress level X up to 30V 150 Ohm test set-up according to IEC/EN 61000-4-6
Max. core temperature:	80 °C
Connector type:	N female
Aperture diameter:	27 mm
Outside diameter:	92 mm
Height:	76 mm
Weight:	1.2 kg

3 Transfer impedance

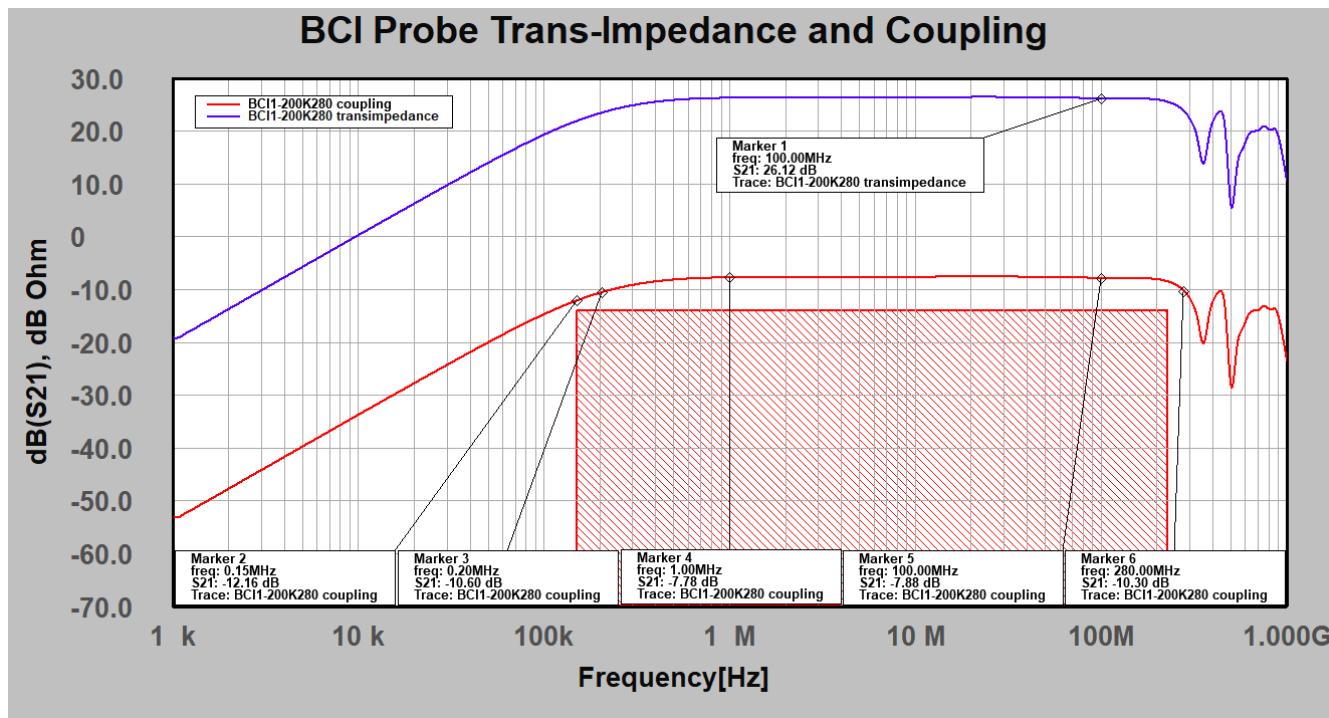


Figure 1: typical insertion loss and transfer impedance: 1 kHz to 1 GHz logarithmic, 50 Ω system (100 Ω loop impedance)

Bulk Current Injection Probe

300 Ohm loop:

Frequency [MHz]	Insertion loss [dB]	Trans-impedance [$\text{dB}\Omega$]	Frequency [MHz]	insertion loss [dB]	Trans-impedance [$\text{dB}\Omega$]
0.01	-41,48	-7,48	30	-16,10	17,90
0.02	-35,56	-1,56	40	-16,09	17,91
0.03	-32,12	1,88	50	-15,95	18,05
0.04	-29,72	4,28	60	-15,89	18,11
0.05	-27,89	6,11	70	-15,78	18,22
0.06	-26,44	7,56	80	-15,80	18,20
0.07	-25,22	8,78	90	-15,68	18,32
0.08	-24,22	9,78	100	-15,70	18,30
0.09	-23,38	10,62	110	-15,64	18,36
0.1	-22,64	11,36	120	-15,55	18,45
0.2	-18,85	15,15	130	-15,51	18,49
0.3	-17,53	16,47	140	-15,39	18,61
0.4	-16,97	17,04	150	-15,20	18,80
0.5	-16,70	17,30	160	-14,99	19,01
0.6	-16,55	17,45	170	-14,71	19,29
0.7	-16,49	17,51	180	-14,48	19,52
0.8	-16,45	17,55	190	-14,27	19,73
0.9	-16,44	17,56	200	-13,97	20,03
1	-16,45	17,55	210	-13,65	20,35
2	-16,43	17,57	220	-13,36	20,64
3	-16,41	17,59	230	-13,11	20,89
4	-16,38	17,62	240	-12,89	21,11
5	-16,38	17,62	250	-12,72	21,28
6	-16,36	17,64	260	-12,57	21,43
7	-16,34	17,66	270	-12,49	21,51
8	-16,31	17,69	280	-12,54	21,46
9	-16,31	17,69	290	-12,84	21,16
10	-16,30	17,70	300	-13,50	20,50
20	-16,21	17,79			

Table 2: Insertion loss and transfer impedance: 10 kHz to 300 MHz, 150 Ω system / 300 Ω loop, typical data

Bulk Current Injection Probe

5 RF forward power requirements


IEC / EN 61000-4-6 specifies following test levels:

Level	Voltage level (e.m.f.)	
	U_0 [V]	U_0 [dB μ V]
1	1	120
2	3	129.5
3	10	140
X*	Special	

* "X" can be any level, above, below or in between the others. The level has to be specified in the dedicated equipment specification

Table 3: test levels, open circuit voltage

The test levels are open circuit voltages set at the EUT port of the coupling devices. For testing of the equipment, this signal is 80 % amplitude modulated with a 1 kHz sine wave to simulate actual threats.

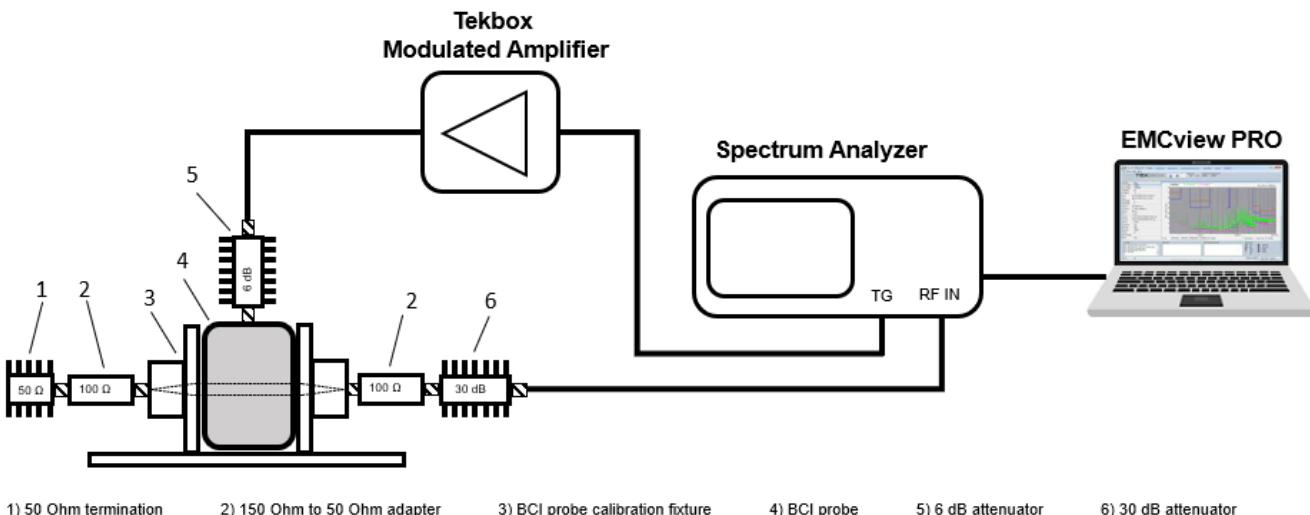

Picture 2: EN 61000-4-6 150Ω system / 300Ω loop calibration set up using EMCview PRO

The test level is set at the output of the 150 Ω to 50 Ω adapter.

The specified test levels are open circuit voltages at the output of the calibration fixture.

The voltages measured during calibration must be multiplied by 3 to allow for the 50 Ω to 150 Ω conversion and again by 2 to reach the open circuit voltage. Hence, the measured voltage

Bulk Current Injection Probe

at the output of the $150\ \Omega$ to $50\ \Omega$ adapter is 1/6th the voltage of the desired stress level. In logarithmic figures, the measured voltage at the output of the $150\ \Omega$ to $50\ \Omega$ adapter is 15.5 dB lower than the open circuit voltage.

Test level	Test voltage e.m.f RMS [V]	Corresponding power at $150\ \Omega$ to $50\ \Omega$ adapter output, RMS [dBm]	Corresponding input power into probe RMS [dBm]	Power amplifier peak power requirement considering 6 dB attenuator and AM modulation [W]
1	1	-2.6	13.9	0.32
2	3	7	23	2.6
3	10	17.4	33.4	28.2

Table 4: PA forward power requirements, $300\ \Omega$ loop, 100 MHz

Table 3 shows the peak power requirements at midband, 100 MHz. The coupling factor for a $150\ \Omega$ system / $300\ \Omega$ loop, measured between probe input to $150\ \Omega$ to $50\ \Omega$ adapter output, has a value of -16 dB at this frequency. The required peak power increases at low frequencies.

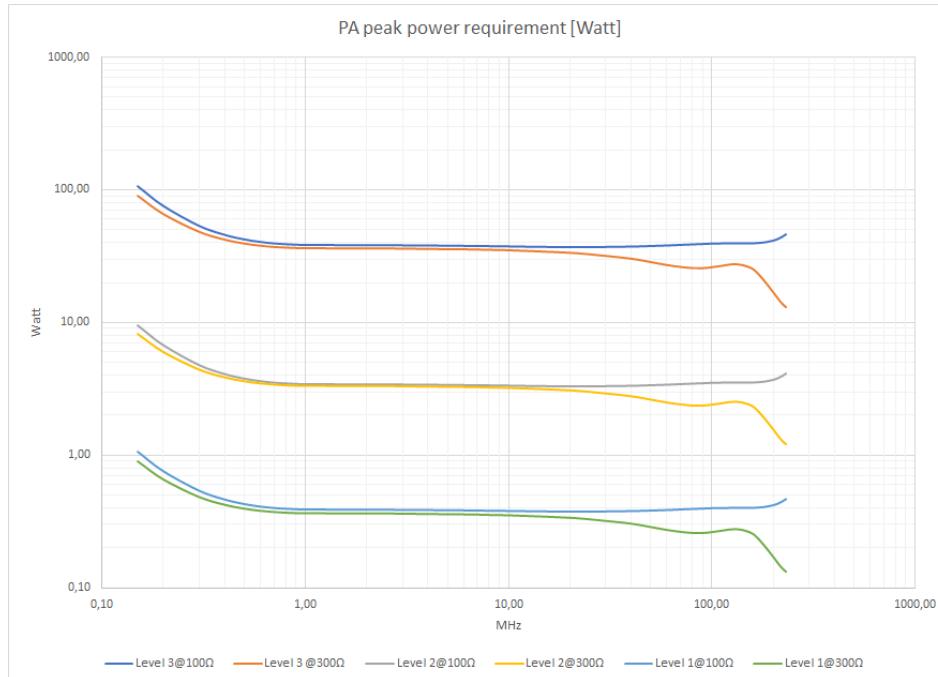


Figure 2: PA peak power requirement (includes 6 dB attenuator and peak power requirement for 80% AM modulation)

Bulk Current Injection Probe

Note that the power is given as RMS Power in Watt. The required peak power of the 80% AM modulated signal is 5.1 dB higher. The probe goes into saturation at stress levels of 30V into a $150\ \Omega$ system / $300\ \Omega$ loop.

Figure 4 shows the core temperature at 30V stress level and 22°C ambient temperature. The measurement time should be limited to 1 hour. At stress level 3, the core takes 4-5 hrs to reach 80°C.


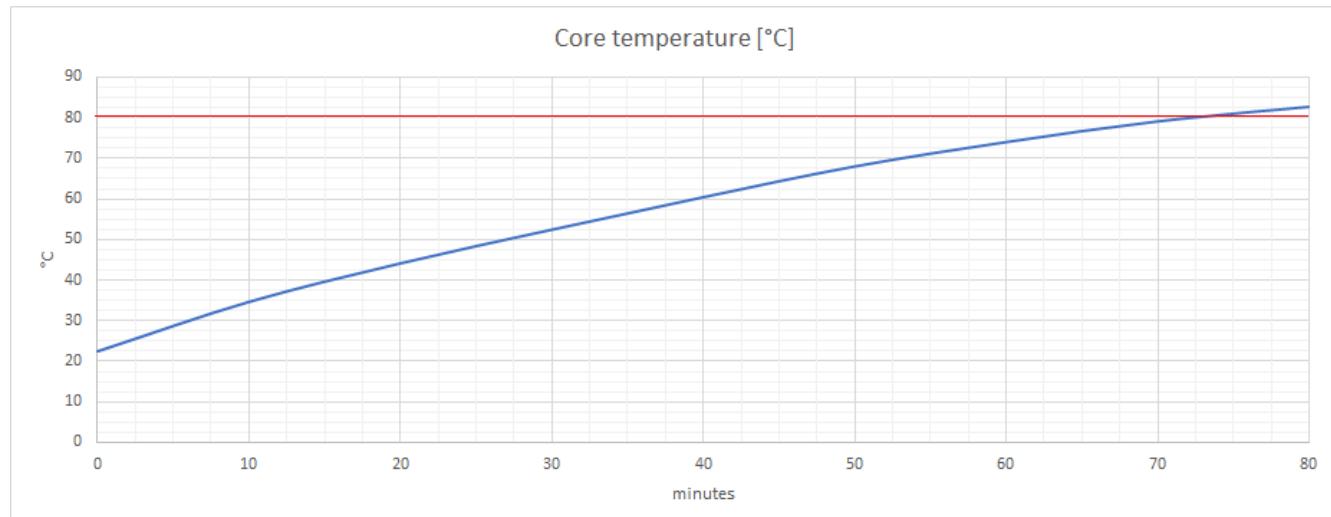


Figure 3: Core temperature increase over time at maximum stress level of 30V

6 Accessories

Tekbox supplies a calibration fixture for the TBBCI1 series of snap on BCI probes:

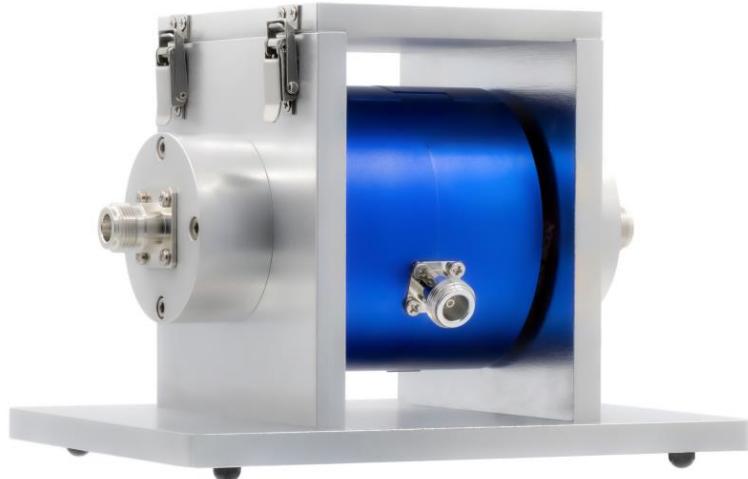

Picture 3: TBBCI1-CAL BCI probe calibration fixture

Bulk Current Injection Probe

In order to create a complete immunity test set-up, Tekbox supplies further accessories such as 150 Ohm to 50 Ohm transitions, attenuators, modulated wideband RF power amplifiers, RF current monitoring probes and EMCview / EMCview PRO software for automated calibration and measurement.

7 Ordering Information

Part Number	Description
TBBCI1-200K280	Snap on BCI probe, beech-wood box, calibration protocol
TBBCI1-CAL	Calibration fixture for TBBCI1 current probe series
TBCDN-50-150	50 Ohm to 150 Ohm adapter, N-male to N-female, 4W
TBATT-6dB-10W	6 dB attenuator, N-male to N-female, 10W
TBATT-6dB-25W	6 dB attenuator, N-male to N-female, 25W
TBATT-6dB-50W	6 dB attenuator, N-male to N-female, 50W
TBATT-6dB-100W	6 dB attenuator, N-male to N-female, 100W
TBATT-30dB-10W	30 dB attenuator, N-male to N-female, 10W
TBATT-30dB-25W	30 dB attenuator, N-male to N-female, 25W
TBATT-30dB-50W	30 dB attenuator, N-male to N-female, 50W
TBATT-30dB-100W	30 dB attenuator, N-male to N-female, 100W
TBMDA5	RF amplifier, 150kHz-400 MHz, 2W, AM/PM modulator
TBMDA6	RF amplifier, 150kHz-250 MHz, 25W, AM/PM modulator
EMCview PRO	EMC software for emission and immunity testing

8 History

Version	Date	Author	Changes
V 1.0	29.9.2022	Mayerhofer	Creation of the preliminary document
V 1.1	13.12.2022	Mayerhofer	Creation of the preliminary document

www.tekbox.com

TekBox Digital Solutions Vietnam Pte. Ltd.

Factory 4, F4, Lot I-3B-1, Saigon Hi-Tech Park, Tan Phu Ward, District 9, Ho Chi Minh City, Vietnam